

DC Electronic Load

PEL-3000AE

QUICK START GUIDE

CWINSTEK PART NO. 82EL-3KEooMC1



SAFETY INSTRUCTIONS

This section contains the basic safety symbols that may appear on the User Manual or on the instrument. For detailed safety instructions and precautions, please see the Safety Instructions chapter in the user manual.

Safety Symbols

These safety symbols may appear in the user manual or on the instrument.

- Warning: Identifies conditions or practices that could result in injury or loss of life.
- Caution: Identifies conditions or practices that could result in damage to the instrument or to other properties.
- DANGER High Voltage
- Attention Refer to the Manual
- Earth (ground) Terminal
- Frame or Chassis Terminal
- Do not dispose electronic equipment as unsorted municipal waste. Please use a separate collection facility or contact the supplier from which this instrument was purchased.

Power Cord for the United Kingdom

When using the instrument in the United Kingdom, make sure the power cord meets the following safety instructions.

NOTE: This lead/appliance must only be wired by competent persons.

WARNING: THIS APPLIANCE MUST BE EARTHED
IMPORTANT: The wires in this lead are coloured in accordance with the following code:

Green/ Yellow: Earth
 Blue: Neutral
 Brown: Live (Phase)



As the colours of the wires in main leads may not correspond with the coloured marking identified in your plug/appliance, proceed as follows:

The wire which is coloured Green & Yellow must be connected to the Earth terminal marked with either the letter E, the earth symbol or coloured Green/Green & Yellow.

The wire which is coloured Blue must be connected to the terminal which is marked with the letter N or coloured Blue or Black.

The wire which is coloured Brown must be connected to the terminal marked with the letter L or P or coloured Brown or Red. If in doubt, consult the instructions provided with the equipment or contact the supplier.

This cable/appliance should be protected by a suitably rated and approved HBC mains fuse: refer to the rating information on the equipment and/or user instructions for details. As a guide, a cable of 0.75mm² should be protected by a 3A or 5A fuse. Larger conductors would normally require 13A types, depending on the connection method used.

Any exposed wiring from a cable, plug or connection that is engaged in a live socket is extremely hazardous. If a cable or plug is deemed hazardous, turn off the mains power and remove the cable, any fuses and fuse assemblies. All hazardous wiring must be immediately destroyed and replaced in accordance to the above standard.

GETTING STARTED

The Getting Started chapter introduces the instrument's main features, appearance, and set up procedure.

Overview

The PEL-3000AE is an economic, standalone, high performance DC electronic load positioned to test a wide range of different power sources. The DC electronic load is fully programmable to simulate anything from basic static loads to complex dynamic loads. The PEL-3000AE is extremely robust and capable of molding to any test environment.

Model Line Up

Model	Operating Voltage (DC)	Current	Power
PEL-3031AE	1V-150V	6A (Low range) 60A (High range)	300W
PEL-3032AE	2.5V-500V	1.5A (Low range) 15A (High range)	300W

Main Features

- Performance**
 - High slew rates of up to 2.5A/ μ s for a fast response speed (PEL-3031AE)
 - High resolution - 16 bit

- Features**
 - 7 operating modes: CC, CV, CR, CP, CC+CV, CR+CV, CP+CV
 - Fully programmable with normal and fast sequences
 - Soft start
 - Dynamic mode
 - OCP, OVP and other protection features
 - Remote sense
 - Integrated meter
 - Rack-mountable

- Interface**
 - USB
 - RS232/RS485
 - GPIB (optional)
 - LAN
 - External voltage or resistance control
 - Rear panel trigger in/out BNC
 - Analog external control

Package Contents and Accessories

Standard Accessories

Item	Part Number
User /Programming Manual CD	
Quick Start Guide (this document)	
Power Cord x1	Region Dependent
Front terminal washers (M6) x2	61SF-062104N1
Remote sense cables, red x1, black x1	GTL-105A

Optional Accessories


Item	Part Number
GPIB cable, 2.0m	GTL-248
USB cable, Type A - Type B	GTL-246
Dust filter	PEL-010
GPIB card	PEL-004
Rack mount frame for PEL-3000A series (JIS)	GRA-414-J
Rack mount frame for PEL-3000A series (EIA)	GRA-414-E
RS-232 cable with DB9 connector to RJ45	GTL-259
RS-485 cable with DB9 connector to RJ45	GTL-260
Serial master cable+ terminator, 0.5 meter.	GTL-261
RS-485 slave cable	GTL-262

This manual contains proprietary information, which is protected by copyright. All rights are reserved. No part of this manual may be photocopied, reproduced or translated to another language without prior written consent of Good Will Corporation.

The information in this manual was correct at the time of printing. However, Good Will continues to improve its products and therefore reserves the right to change the specifications, equipment, and maintenance procedures at any time without notice.

Good Will Instrument Co., Ltd. No. 7-1, Jhongsing Rd., Tucheng Dist., New Taipei City 236, Taiwan.


Front Panel

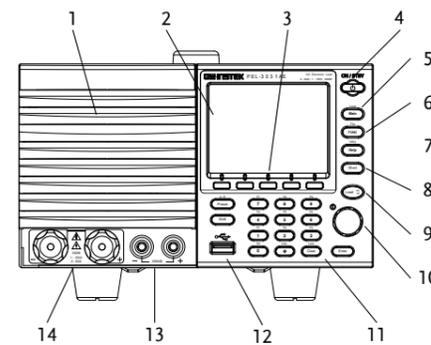

Description

- | | |
|---|-------------------------------------|
| 1. Air inlet | 2. LCD Display |
| 3. Function keys | 4. Power key |
| 5. Main/Local key | 6. FUNC/File key |
| 7. Help/Utility key | 8. Short key |
| 9. Load On/Off | 10. Scroll wheel |
| 11. Number pad, Clear/Lock and Enter keys | 12. USB port, Preset and Shift keys |
| 13. Sense-, Sense+ terminals | 14. Input terminals |


Rear Panel

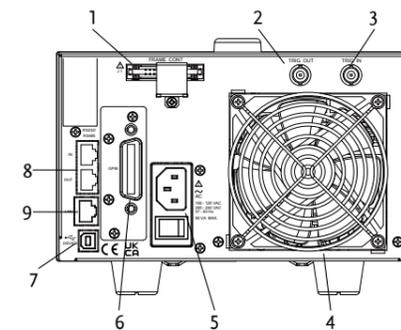

Description

- | | |
|----------------------------|---------------------|
| 1. J1 Frame control ports | 2. TRIG OUT BNC |
| 3. TRIG IN BNC | 4. Exhaust fan |
| 5. Power socket and switch | 6. GPIB (optional) |
| 7. USB device port | 8. RS232/RS485 port |
| 9. LAN port | |

Display Overview

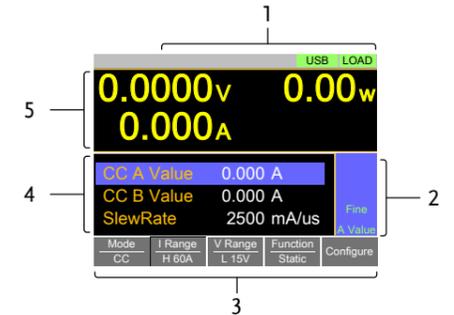



Description

- | | |
|----------------------------|---------------------------|
| 1. Main frame status panel | 2. Operation status panel |
| 3. Soft keys | 4. Setting area |
| 5. Measurement area | |

First Time Use Instructions

Use the following procedures when first using the PEL-3000AE to power up the instrument, restore the factory default settings and check the firmware version. Lastly, the Conventions section will introduce you to the basic operating conventions used throughout the user manual.

Power Up

1. Insert the AC power cord into the power socket.
2. Turn the power switch on from the rear panel. 
3. If the unit doesn't turn on, press the ON/STBY key on the front panel.
 - The ON/STBY key will go from standby (red) to ON (green).
4. The unit will show the splash screen and then load the settings from when the unit was last powered down.

Load Default Settings

When first using the PEL-3000AE, recall the factory default settings to ensure the unit is in a known state. See the user manual for a list of the default settings.


1. Press **Shift** + **File** + **FUNC**.
2. Select *Media/Default* [F1].
3. Select *Factory Default* [F2].
4. Press *Factory Default* [F2] again to confirm.

Entering Alphanumeric Characters

When renaming files, creating memos or notes, you will be required to enter alphanumeric characters when the character entry screen appears.

- Only alphanumeric characters as well as space [], underscore [_] and minus [-] characters are allowed.

1. Use the scroll wheel to move the cursor to the desired character.



2. Press the **Enter** key or *Enter Character*[F1] to select a character.
3. To delete a character, press *Back Space*[F2].
4. To save the file name or memo, press *Save*[F3].

Updating the Firmware

The PEL-3000AE allows the firmware to be updated by end-users. Before using the PEL-3000AE, please check the GW Instek website or ask your local distributor for the latest firmware. Before updating the firmware, please check the firmware version.

View Firmware Version

1. Press **Shift** + **Utility** + **Help**.
2. Select *System/Info*[F1].
3. The system information is listed in the display.
 - Model: PEL-303XAE
 - Serial Number: XXXXXXXX
 - Firmware Ver.: 1.XX
 - GW Instek website address.

Firmware update

1. Press **Shift** + **File** + **FUNC**.
2. Select *USB* with the *Media* [F1] soft-key.
3. Press the *File Utility* [F5] soft-key.
4. Select the *.UPG upgrade file and press *Select*[F1] twice. Once to select the file and once to confirm.
5. Wait for the update to complete and reset the power.

Warning Do not turn the load generator off or remove the USB memory when the firmware is being read or upgraded.

SPECIFICATIONS

The following are the basic specifications for the PEL-3000AE. For detailed specifications, please see the user manual.


Overall				
Model	PEL-3031AE	PEL-3032AE		
Power	300W	300W		
Range	Low	High	Low	High
Voltage	1-150V	2.5-500V		
Current	0-6A	0-60A	0-1.5A	0-15A
Min. Operating Voltage(dc)	1V-6A	1V-60A	2.5V-1.5A	2.5V-15A
Static Mode				
Range	Low	High	Low	High
Constant Current Mode				
Range	0-6A	0-60A	0-1.5A	0-15A
Setting Range	0-6.12A	0-61.2A	0-1.53A	0-15.3A
Resolution	0.2mA	2mA	0.05mA	0.5mA
Accuracy	(T ¹) ± (0.1% of set + 0.1% of F.S) + Vin/500kΩ		(T ¹) ± (0.1% of set + 0.2% of F.S) + Vin/500kΩ	
	(Full scale of High range)		(Full scale of High range)	
Constant Resistance Mode				
Range	60S-0.002S	6S-0.0002S		
	(0.01666Ω-500Ω)	(0.16666Ω-5kΩ)		
	(300W/15V)	(300W/50V)		
	6S-0.0002S	0.6S-0.00002S		
	(0.1666Ω-5kΩ)	(1.6666Ω-50kΩ)		
	(300W/150V)	(300W/500V)		

Conventions

The following conventions are used throughout the user manual. Read the conventions below for a basic grasp of how to operate the PEL-3000AE menu system using the front panel keys.

Soft-menu keys

The F1 to F5 function keys at the bottom of the display correspond directly to the soft-menu keys on top.

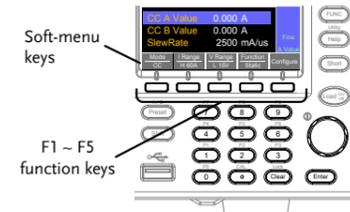


Select Sub Menu



Pressing this type of soft-menu key will enter a submenu.

Setting Range	60S-0.002S (0.01666Ω-500Ω) (300W/15V)	6S-0.0002S (0.16666Ω-5kΩ) (300W/50V)		
Resolution	0.002S(15V)	0.0002S(50V)		
Accuracy	(T ¹) ± (0.3% of set + 0.6S) + 0.002mS	(T ¹) ± (0.3% of set + 0.06S) + 0.002mS		
Constant Voltage Mode				
Range	1-15V	1-150V	2.5-50V	2.5-500V
Setting Range	0-15.3V	0-153V	0-51V	0-510V
Resolution	0.5mV	5mV	1mV	10mV
Accuracy	(T ¹) ± (0.1% of set + 0.1% of F.S) (Full scale of Low range)		(T ¹) ± (0.1% of set + 0.1% of F.S) (Full scale of High range)	
Input Current Variation *2	12mV	40mV		
Constant Power Mode				
Range	3-30W (6A)	30-300W (60A)	3-30W (1.5A)	30-300W (15A)
Setting range	0-30.6W	0-306W	0-30.6W	0-306W
Resolution	1mW	10mW	1mW	10mW
Accuracy	(T ¹) ± (0.6% of set + 1.4% of f.s (Full scale of H range)) + Vin2/500kΩ			
*1: If the ambient temperature is over 30°C or below 20°C, then T = ± t-25°C × 100ppm/°C × Set. If the ambient is in the range of 20 ~ 30°C, then T = 0 (t is the ambient temperature)				
*2: With respect to a change in the current of 10% to 100% of the rating at an input voltage of 1V or 2.5V (during remote sensing).				
Dynamic Mode				
Range	Low	High	Low	High
General				
T1 & T2	0.05mS - 30mS / Res : 1uS			

Toggle Parameter or State



This type of soft-menu icon has the function/item on the top of the label and the selected setting or mode on the bottom of the label.

Repeatedly press the associated function key (F1-F5) to cycle through each setting.

For some parameters, a popup window will also appear. Selection of the setting is the same. Repeatedly pressing the relevant function key (F1-F5) will cycle through each setting.

Parameter Input

The scroll wheel, Enter key and number pad can be used to edit parameter values.


1. Use the scroll wheel to move the cursor to the desired parameter.
 - A scroll bar is shown when there are additional parameters off-screen.



2. Press the **Enter** key to select the parameter.
3. Then use the number pad* or scroll wheel** to edit the parameter value.

	30mS - 30S / Res : 1mS			
Accuracy	1uS / 1mS	± 200ppm		
Slew Rate	0.001-	0.01-	0.25-	2.5-
(Accuracy 10%)	0.25A/uS	2.5A/uS	62.5mA/uS	625mA/uS
Slew Rate	0.001A/	0.01A/uS	0.25mA/	2.5mA/
Resolution	uS	uS	uS	uS
Slew Rate	± (10% + 15us)		± (10% + 15us)	
Accuracy of Setting*1				
Constant Current Mode				
Range	Low	High	Low	High
Current	0-6A	0-60A	0-1.5A	0-15A
Setting range	0-6.12A	0-61.2A	0-1.53A	0-15.3A
Current	0.2mA	2mA	0.05mA	0.5mA
Resolution	Current Accuracy ± 0.8% F.S.			
Constant Resistance Mode				
	60S-0.002S	6S-0.0002S		
	(0.01666Ω-500Ω)	(0.16666Ω-5kΩ)		
	(300W/15V)	(300W/50V)		
Resistance	6S-0.0002S	0.6S-0.00002S		
	(0.1666Ω-5kΩ)	(1.6666Ω-50kΩ)		
	(300W/150V)	(300W/500V)		
Setting range	60S-0.002S	6S-0.0002S		
	(0.01666Ω-500Ω)	(0.16666Ω-5kΩ)		
	(300W/15V)	(300W/50V)		
	6S-0.0002S	0.6S-0.00002S		
	(0.1666Ω-5kΩ)	(1.6666Ω-50kΩ)		
	(300W/150V)	(300W/500V)		
Resistance	3000 Steps	3000 Steps		
Accuracy	± (1%set + 0.6S)+0.002mS	± (1%set + 0.06S)+0.002mS		

*1: Time to reach from 10% to 90% when the current is varied from 2% to 100% (20% to 100% in L range) of the rated current.




Clearing a Value*

*When editing a parameter with the number pad, pressing the **Clear** key will restore the parameter to the previous value.

Coarse/Fine Adjustment**

**When a parameter is highlighted (step 3 above) pressing the scroll wheel will toggle the scroll wheel resolution between fine and coarse.

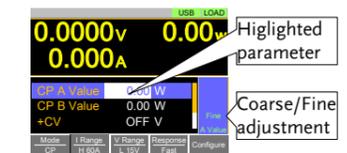

Note: There is a second method of fine adjustment that allows you to edit parameters one digit value at a time using the scroll wheel. This is called Cursor mode. Please see the user manual for more information.

Declaration of Conformity

We **GOOD WILL INSTRUMENT CO., LTD.** declare that the CE marking mentioned product satisfies all the technical relations application to the product within the scope of council: Directive: EMC; LVD; WEEE; RoHS The product is in conformity with the following standards or other normative documents:

© EMC	
EN 61326-1	Electrical equipment for measurement, control and laboratory use -- EMC requirements
Conducted & Radiated Emission EN 55011 / EN 55032	Electrical Fast Transients EN 61000-4-4
Current Harmonics EN 61000-3-2 / EN 61000-3-12	Surge Immunity EN 61000-4-5
Voltage Fluctuations EN 61000-3-3 / EN 61000-3-11	Conducted Susceptibility EN 61000-4-6
Electrostatic Discharge EN 61000-4-2	Power Frequency Magnetic Field EN 61000-4-8
Radiated Immunity EN 61000-4-3	Voltage Dip/ Interruption EN 61000-4-11 / EN 61000-4-34
© Safety	
EN 61010-1 :	Safety requirements for electrical equipment for measurement, control, and laboratory use - Part 1: General requirements

GOODWILL INSTRUMENT CO., LTD.
No. 7-1, Jhongsing Road, Tucheng District, New Taipei City 236, Taiwan
Tel: +886-2-2268-0389 Fax: +886-2-2268-0639
Web: <http://www.gwinstek.com> Email: marketing@goodwill.com.tw
GOODWILL INSTRUMENT (SUZHOU) CO., LTD.
No. 521, Zhujiang Road, Snd, Suzhou Jiangsu 215011, China
Tel: +86-512-6661-7177 Fax: +86-512-6661-7277
Web: <http://www.instek.com.cn> Email: marketing@instek.com.cn
GOODWILL INSTRUMENT EURO B.V.
De Run 5427A, 5504DG Veldhoven, The Netherlands
Tel: +31-(0)40-2557790 Fax: +31-(0)40-2541194
Email: sales@gw-instek.eu